

For the protection of your employees: Testing of protective masks in one minute before daily use.



*Offer includes testing at Palas with test rig PMFT 2000 (with oil or NaCl) for the determination of penetration for particle sizes of 300 nm to 3 µm (oil) or from 300 nm to 5 µm (NaCl).


Description

The Mas-Q-Check was developed by Palas to subject protective masks to a quick, simple and yet meaningful test before use. A particle counting measurement device is used, which is able to detect efficiencies in the size range of viruses and bacteria. The system can also be used for training purposes as it immediately shows the efficiency of protective masks. Two versions are available:

- **Mas-Q-Check Basic** with a volume flow of 9.5 l/min
- **Mas-Q-Check Professional** with a volume flow of 95 l/min (pictured)

Accessories:

Mas-Q-Box consists of an aerosol chamber with aerosol generator for oil and salt aerosols (we recommend this accessory in combination with Mas-Q-Check Professional). The head with the installed mask is inserted into the aerosol chamber. The PAG 1000 aerosol generator is used to introduce the aerosol into the chamber. In this way, the degree of separation of the mask at the head can be determined with a defined aerosol. This enables the separation efficiency of everyday masks to be determined quickly and easily in accordance with the new EU directive CAW 17553.

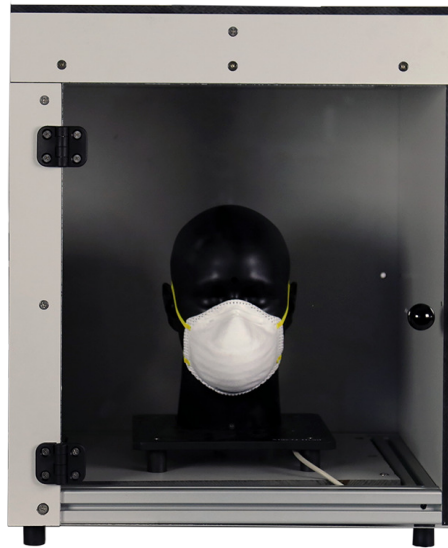**Functionality:**

The mask is placed on the test head before use. Using a high-resolution aerosol spectrometer, the particle contamination (size and quantity) in the ambient air is measured. Afterwards the device switches automatically and determines the value of the particle contamination behind the protective mask. This can be repeated automatically several times. The ratio of the two measured values is used to determine the degree of protection of the protective mask. A simple display immediately shows whether the mask can be used.



Mas-Q-Check basic

manual sampling

FFP classes

protective rating

expert user menu

shut down

menu

measurement stopped...




20:35:48
05/04/2020



Mas-Q-Check protection rating

start

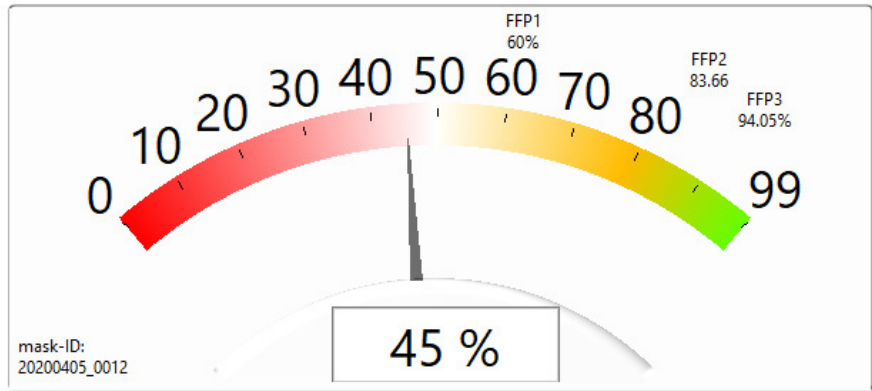

print

menu

measurement stopped...



20:40:01
05/04/2020

Degree of protection:

The degree of protection provided by a respirator depends on the filtration effect of the mask material as well as the correct fit on the head. Leakage can occur (i.e. air passes the material and enters behind the mask unfiltered), which affects the protective effect. means of the test on the standard head with the Mas-Q-Check, both effects are simulated simultaneously and the real protective effect of the mask against particles in the outside air is measured. The result shows the degree of protection in

comparison to the FFP Class of the mask on the test head. Optional on display is the efficiency for different particle sizes. SO the degree of protection may vary with regard to the particle size.

Quality of the measurement:

The Mas-Q-Check works in suction mode with a volume flow of either 9.5 l/min or 95 l/min, defined according to EN149 or EN143, which corresponds to the maximum human breath. The measurement of particle contamination in the room and after the breathing mask is carried out by means of a high-resolution aerosol spectrometer, which precisely measures particle sizes from 140 nm to 1 μm . Thus, the protective effect of viruses is also determined.

the Mas-Q-Check, safe on-site testing of respiratory masks is therefore possible automatically within 1 minute.

Benefits

- Self-explanatory operation
- Quick easy and exact measurement of the degree of protection of masks on site
- Quality control of masks in daily use
- Reral evaluation of the degree of protection from filtration efficiency and leakage combined.
- Highly resolved measurement result in the range of 140 nm up to 1 μm
- Fully automated test
- Evaluation of the degree of protection in comparison to the FFP class, optional display with regard to particle size
- Clear distinction of protection degree in the size range of viruses and bacteria and above

Datasheet

<i>Parameter</i>	<i>Description</i>
Measurement range (size)	0.14 – 10 µm
Measuring principle	Optical light-scattering
Measurement range (number C_N)	0 – 20,000 particles/cm ³
Data acquisition	Digital, 20 MHz processor, 256 raw data channels
Power consumption	approx. 200 W
User interface	
	Touch screen, 800 • 480 pixel, 7"
Reported data	Protection class filter mask
Volume flow (clean air)	9.5 l/min, 95 l/min

Applications

- Confirmation of the degree of protection of masks
- Confirmation of the protection of employees working in medical environment
- Training to show the correct use of masks with direct measurement of the degree of protection
- Evaluation of the real degree of protection in comparison of the FFP Class

Palas GmbH
Partikel- und Lasermesstechnik
Greschbachstrasse 3 b
76229 Karlsruhe
Germany

Managing Partner:
Dr.-Ing. Maximilian Weiß
Commercial Register:
register court: Mannheim
company registration number: HRB 103813
USt-Id: DE143585902



Contact: E-Mail: mail@palas.de Internet: www.palas.de Tel: +49 (0)721 96213-0 Fax: +49 (0)721 96213-33