



DESCRIPTION

The PMFT 1000 tests respirators better than the standards EN 149/EN 13274-7 with additional accurate analysis of filter mask efficiency for SARS-CoV-2 (size approximately 120 nm to 160 nm). Both total photometric penetration and fractional efficiency are tested e.g., the efficiency in the whole size range respectively the particle size-dependent penetration.

In addition, the PMFT 1000 meets the requirements for respirators specified by the **CCF (Covid Certified Filter) quality seal**¹.



The PMFT 1000 is equipped with aerosol generators for measuring penetration with oil and salt. Measurement procedures for quick quality control (short test) or for testing according to standard (exposure test) are supplied.

Operation and automatic printout of the measurement results are therefore easy even for inexperienced users.

¹CCF-Siegel: <https://www.ccf-quality.com/>


The measurement of total penetration and penetration via particle size is carried out with the high-precision Promo 1000 aerosol photometer.

The size distribution of the test aerosol according to the standard is as follows:

EN 149

Oil: Media diameter 290 nm | Geom. standard deviation 1.85


Salt: Media diameter 70 nm | Geom. standard deviation 2.5

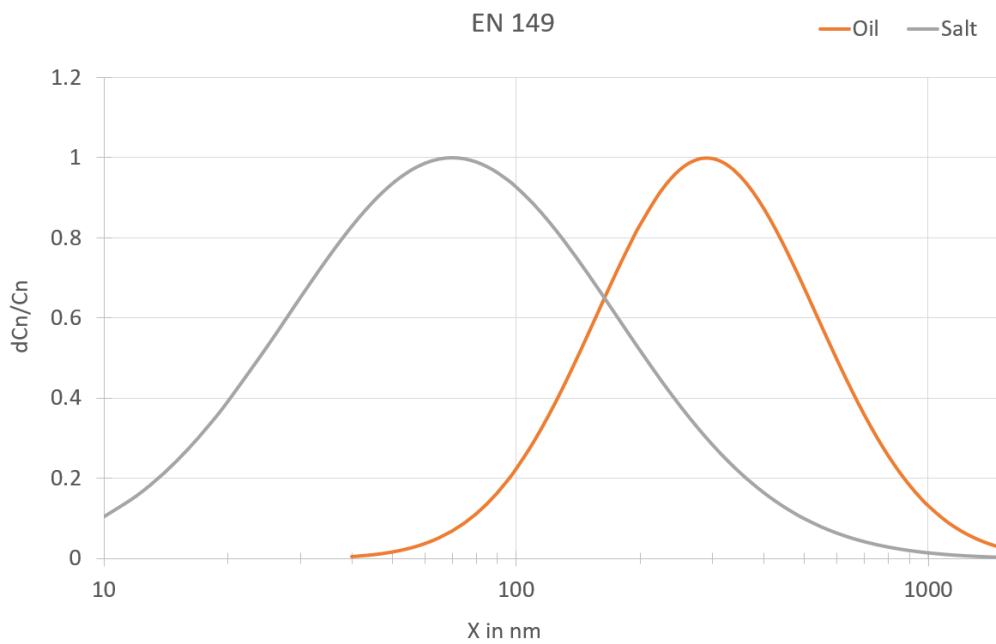

42 CFR 84 / GB 2626

Oil: Media diameter 200 nm | Geom. standard deviation 1.6

Salt: Media diameter 55 nm | Geom. standard deviation 1.86

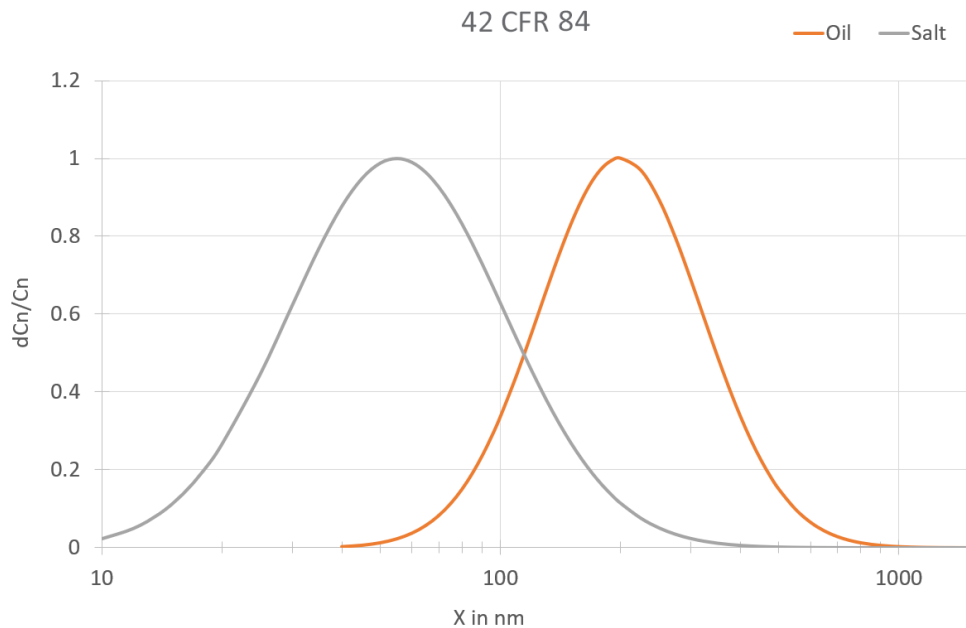

Based on the measurement of particle penetration via particle size, the PMFT can also be used to view the tolerances in the particle size distribution according to EN 13274-7 as min. / max. penetration values. In addition, comparative values to other manufacturers are possible (option).

Comparison of EN149 penetrations

Test information

| | | | |
|----------|----------|------------|----------|
| Operator | Date | Time | Version |
| MKS | 12.42.05 | 26.04.2021 | 1.10.3.0 |


Basic information

| | |
|---------------|-----------------------|
| Script | Efficiency Test (oil) |
| Aerosol | Oil |
| Main air | 95.05 l/min |
| Generator air | 2.19 l/min |

Mask information

| | |
|-----------|-----------------------|
| Mask ID | 14087_20210426_124205 |
| Mask los | |
| Mask type | FFP2 / x / x |

Penetration [%]

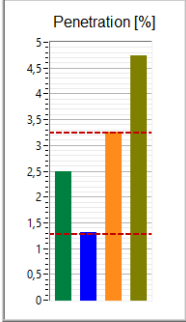


Result

| | EN149 min | EN149 max | PMFT | DMT | MF1 | MF2 |
|------------------------------|-----------|-----------|---------|------|---------|---------|
| Penetration [%] | 1.27 | 3.24 | 2.49 | 1.30 | 3.26 | 4.75 |
| Based on X _g [µm] | 0.45 | 0.29 | 0.29 | 0.29 | 0.185 | 0.13 |
| Based on Sigma | 2.2 | 1.6 | 1.85 | 1.85 | 2 | 1.9 |
| Rating | P_Ph_45 | P_Ph_45 | P_Ph_45 | P_m | P_Ph_45 | P_Ph_45 |

exit

The comparison with other standards (42CFR84/NIOSH) is also easy with the 42CFR84 upgrade KIT.

Penetration of reference sheets PMFT to NIOSH approved
Mask Testing system; NaCl at 85 l/min

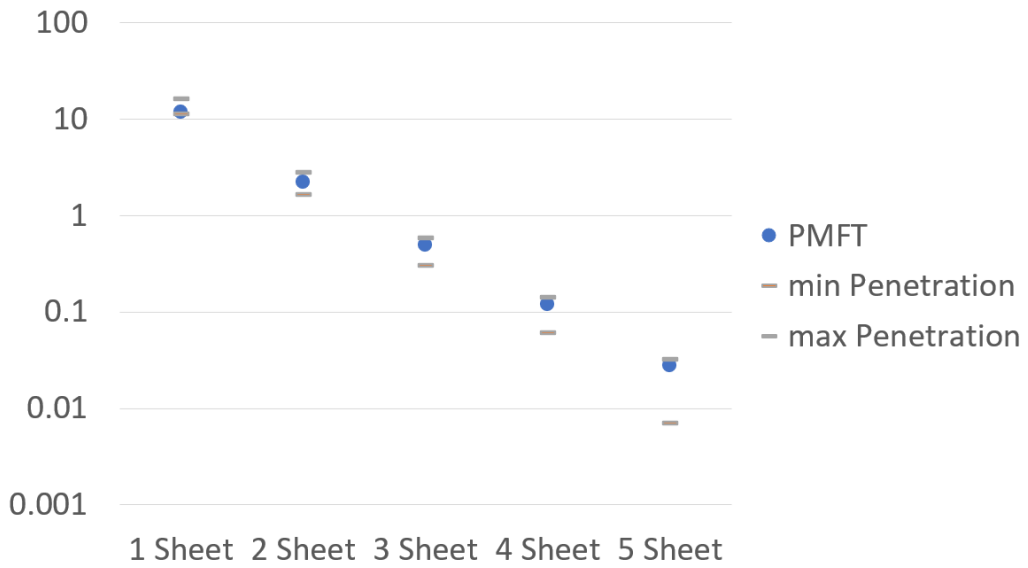

BENEFITS

- Test rig working principle better than EN 149 and EN 13274-7
- Equivalent to GB 2626, 42 CFR 84 and ASTM 2299-3 by additional software option
- Test of community masks equivalent to CWA 17553
- Meets the requirements for respirators specified by the **CCF (Covid Certified Filter) quality seal²**
- Includes two aerosol generators for oil and NaCl
- Testing of fractional efficiency, e.g., efficiency in whole size range of 100 nm up to 3 μm
- Exact analysis of filter and filter mask efficiency for SARS-CoV-2 (size approx. 120 nm up to 160 nm) in the size range between 100 nm and 180 nm we have eight size channels
- Future proof: Works with any kind of aerosol without adjustments
- Further measurement of differential pressure, e. g., as well within different face velocities to simulate measurement of breath resistance
- Face velocity adjustable between 1.5 – 70 cm/s
- Product capable of fast quality assurance **and** continuous optimization in RD (display of size distribution)
- Individual face mask adapter for your product
- Attractive two years maintenance package for availability of test rig

The software extension additionally offers:

- Display of penetration results of the entire tolerance range of the size distribution according to EN 13274-7
- Allows the comparison of different test institutes and test systems
- Facilitates certification
- Shows wide range of standards. Depending on the test operation – i.e., particle size distribution of the test aerosol – one and the same mask can perform very well or fail the test

²CCF-Siegel: <https://www.ccf-quality.com/>

DATASHEET

| | |
|---------------------------------------|--|
| Measuring range (total penetration) | 0.0005 - 100 % |
| Measurement range (size) | 0.1 – 40 μm |
| Volume flow | 1 – 27 m^3/h - pressurized operation |
| Installation conditions | +10 – +40 °C |
| Inflow velocity | 1.5 – 70 cm/s (others on request) |
| Differential pressure measurement | 0 – 1,200 Pa |
| Aerosols | Salts (e.g. KCl, NaCl), liquid aerosols (e.g. DEHS), latex particles (PSL) |
| Compressed air supply | 6 – 8 bar |
| Test area of the medium | 100 cm^2 |
| Dilution factor | 1:27 |
| Power supply | 115 – 230 V, 50/60 Hz |
| Test conditions according to standard | +19 – +23 °C |
| Dimensions | Approx. 1,800 • 600 • 900 mm (H • W • D) |

APPLICATIONS

- Development and production monitoring of half masks
- Test of total penetration for respiratory masks
- Exact analysis of filter mask efficiency for e.g., Coronavirus



Mehr Informationen:
<https://www.palas.de/product/pmft-1000>

| | EN 149 | EN 13274-7 | EN 13274-7 | GB 2626 | GB 2626 | 42 CFR 84 | 42 CFR 84 |
|---------------------------|----------------|-------------------------------|--------------------------------|--|--|--|---------------------------------------|
| Aerosol | see EN 13274-7 | NaCl | PaO | NaCl | PaO/DOP | NaCl | DOP |
| Mean diameter | see EN 13274-7 | 0.06 – 0.1 μm | 0.29 – 0.45 μm | 0.055 – 0.095 μm | 0.165 – 0.205 μm | 0.055 – 0.095 μm | 0.165 – 0.205 μm |
| Standard deviation | see EN 13274-7 | 2 – 3 | 1.6 – 2.2 | < 1.86 (by additional software module) | < 1.6 (by additional software module) | < 1.86 (by additional software module) | < 1.6 (by additional software module) |
| Concentration | see EN 13274-7 | 4 – 12 mg/m^3 | 15 – 25 mg/m^3 | < 200 mg/m^3 | (50 mg/m^3) < 200 mg/m^3 | < 200 mg/m^3 | < 200 mg/m^3 |
| Discharge | - | - | - | required | required | required | required |
| Air flow | see EN 13274-7 | 95 l/min | 95 l/min | 85 \pm 4 l/min | 85 \pm 4 l/min | 85 \pm 4 l/min | 85 \pm 4 l/min |
| Temperature | see EN 13274-7 | 22 \pm 3 $^{\circ}\text{C}$ | - | 25 \pm 5 $^{\circ}\text{C}$ | 25 \pm 5 $^{\circ}\text{C}$ | 25 \pm 5 $^{\circ}\text{C}$ | 25 \pm 5 $^{\circ}\text{C}$ |
| Rel. humidity | see EN 13274-7 | < 40 % | - | 20 – 40 % (by compressed air) | - | 20 – 40 % (by compressed air) | 20 – 40 % (by compressed air) |
| Measurement device | see EN 13274-7 | Sodium flame photometer | Light scattering photometer | particle detector | particle detector | Light scattering photometer | Light scattering photometer |
| Measuring time | see EN 13274-7 | 30 s | 30 s | lowest eff. during loading | lowest eff. during loading | lowest eff. during loading | lowest eff. during loading |
| Pause time | see EN 13274-7 | 180 s | 180 s | lowest eff. during loading | lowest eff. during loading | lowest eff. during loading | lowest eff. during loading |
| Exposition | 120 mg | 120 mg | 120 mg | 200 \pm 5 mg | 200 \pm 5 mg | 200 \pm 5 mg | 200 \pm 5 mg |
| PMFT remarks | O.K. | O.K. | O.K. | O.K. with upgrade KIT | O.K. with upgrade KIT | O.K. with upgrade KIT | O.K. with upgrade KIT |

Table 2: Overview of standards for face mask penetration testing